


Oticon NoWax - Replacement procedure

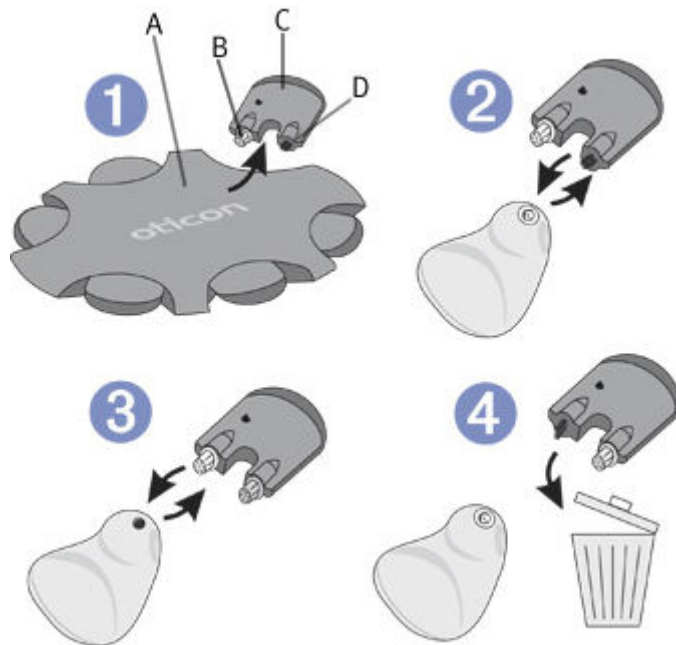

1. Remove the tool (C) from the shell (A). The tool has two arms, one with the new filter (B) and one with the removal tool (D)
2. Push the removal tool into the existing wax filter and remove the used filter from the hearing aid
3. Push the new filter into the hearing aid
4. Discard the used tool